


Lab-on-a-Chip Part 2 – Detection Methods

Prof. Steven S. Sallierman, <http://sallierman.umn.edu/>

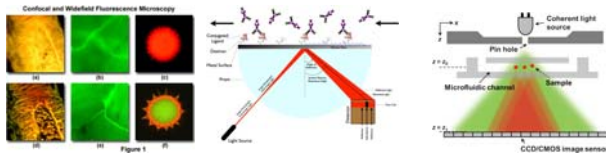


Topics

- Electrochemical Detection
 - Capillary electrophoresis.
 - Electrochemical impedance spectroscopy (EIS) – See Gamry Instrument article
- Optical Detection
 - Conventional Off-Chip or “Free-Space”
 - Absorbance Detection
 - Fluorescence Detection
 - Chemiluminescence
 - Surface Plasmon Resonance
 - Surface Enhanced Raman Spectroscopy
 - On-Chip Methods
 - Frequency Specific LEDs
 - Absorbance Spectroscopy
 - Fluorescence
 - Chemiluminescence
 - Optical Waveguides
 - Surface Plasmon Resonance
 - Interferometry
 - Holography

Steven S. Sallierman

Glass and Polymer Based Devices

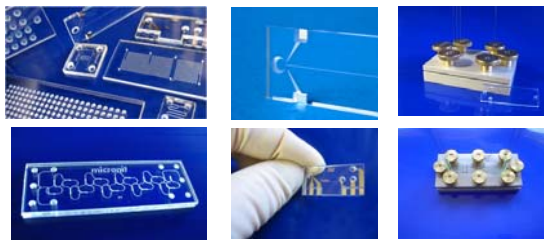

Steven S. Sallierman



Images courtesy of Micronit

Positive "Downscaling" Effects

- Reduced sample and reagent volumes.
- Ten fold reduction in length scale.
- Laminar flow (low Reynolds numbers).
- Improved mass flow by diffusion.
- Harvesting electrokinetic effects
- The *surface-to-volume ratio* (SVR) may increase by a factor of more than *ten thousand* during downscaling and solute/wall interactions become dominant.

Steven S. Sallterman

Consider Capillary Electrophoresis




- Sample introduction and electrophoretic separation are accomplished in each of two crossing channels.
- Sample is driven through the short sample channel across the separation channel by application of a potential, and
- The introduced sample "plug" (nanoliter volume) is then electrophoretically separated by application of another potential.

Steven S. Sallterman

Guber AE et al., Microfluidic lab-on-a-chip systems based on polymers – fabrication and application," Chemical Engineering Journal 101(1-3), pp 447-453 (2004). Image courtesy of Microfluidics

Capillary Electrophoresis...




- High voltage along the length of the capillary separates the analytes and drives them toward the detection electrodes.
- A constant potential is applied with a potentiostat to the detection electrodes.
- As each species passes, a change in current or conductivity between the detection electrodes is detected.

Steven S. Sallterman

Gençoğlu, A. and Adrienne R. Minerick, "Electrochemical detection techniques in micro- and nanofluidic devices," Microfluid. Nanofluid. (2014) 17:791–807


Video of Capillary Electrophoresis...

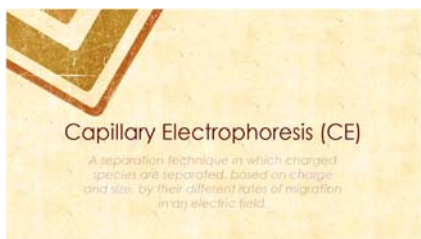

Steven S. Sallerman

<https://youtu.be/wStV1rFjH0o>

Recall Electrochemical Impedance Spectroscopy (EIS)...



(For a more detailed discussion of EIS see the Gamry Industries article.)

- Three-electrode electrochemical cell. (WE = Working Electrode, CE = Counter Electrode, RE = Reference Electrode & V = Voltage).
- On the left, a small AC voltage is applied across the WE and RE of a three-electrode electrochemical cell.
- Current is then measured from the WE to the CE, and varies with frequency and the analyte concentration.

a) Giering, A. and Adrienne R. Miseric, Electrochemical detection techniques in micro- and nanofluidic devices. *Microfluid. Nanofluid.* (2014) 17:781-807
b) Fan, L., Zhao, G., Shi, H., Liu, M. Li, Z. (2013) A highly selective electrochemical impedance spectroscopy-based aptasensor for sensitive detection of acetaminophen. *Biosens. Bioelectron.* 43:12-18. doi:10.1016/j.bios.2012.11.033

Steven S. Sallerman


What is Impedance?

- **Impedance (Z)** – Total opposition a device or circuit offers to flow of an *alternating current* at a given *frequency*.
 - Units are in ohms
 - Complex quantity graphically shown on a vector plane (real and imaginary parts): $R + jX$ where R is *resistance* and X *reactance*

Steven S. Sallerman

Recall Aptamers...

- Aptamers are **artificial nucleic acid ligands** that can be generated against amino acids, drugs, proteins and other molecules.
- Function similar to **antibodies**.
- **Applications:**
 - Therapeutics,
 - Target validation,
 - Drug screening,
 - Affinity separation,
 - Diagnostics and biosensors.




Steven S. Sallterman

Image courtesy of Archemix


Example of an EIS Implementation...

- Typically applications depend on a specific binding event between the analyte and a recognition element (e.g., enzyme, DNA probe, and antigen), which form a surface layer on the detection electrode, bound directly or through a linker molecule, as shown.
- Shown is modification of an Au working electrode surface for selective detection of the analyte acetamiprid via specific analyte-aptamer binding.



Steven S. Sallterman

- The bare Au surface plot is shown leftmost. The spectra changes as the surface is functionalized with Au nanoparticles, aptamer, and a blocking agent to block nonspecific binding sites on the aptamer molecule.

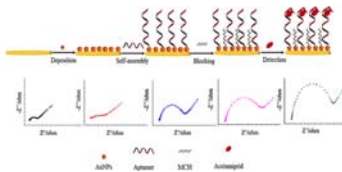

- Nyquist plots (impedance in ohm). The extent of the shift in EIS response (two final spectra) upon analyte binding, is a function of the analyte concentration. [See also Bode plots.]

a) Genozogu, A and Adrienne R. Miserick. Electrochemical detection techniques in micro- and nanofluidic devices. *Microfluid. Nanofluid.* (2014) 17:781–807
 b) Fan, L., Zhao, Q., Shi, H., Liu, M. J. Z. (2013) A highly selective electrochemical impedance spectroscopy-based aptasensor for sensitive detection of acetamiprid. *Biosens. Bioelectron.* 43:12–18. doi:10.1016/j.bios.2012.11.033

Steven S. Sallterman

Optical Detection: Off-Chip


- Absorbance Detection
- Fluorescence Detection
- Chemiluminescence
- Surface Plasmon Resonance
- Localized Surface Plasmon Resonance (LSPR) Spectroscopy (*electromagnetic-field enhancement that leads to surface enhanced Raman Scattering and other surface-enhanced processes*)

Steven S. Sattlerman

Gai, Hongwei, Yongjun Li, and Edward S. Yeung. 2011. Optical Detection Systems on Microfluidic Chips. *Microfluidics: Technologies and Applications* 304, 171-201.

Absorbance Detection


- UV/Vis light is used for absorption spectroscopy.
- Absorption spectra are related to the structure and concentration of the analyte and are based on the capability of samples to attenuate the incident electromagnetic radiation at various wavelengths.



Steven S. Sattlerman

Introducing Fluorophores...

- A *fluorophore* is a fluorescent chemical compound that may re-emit light upon light excitation.
- Fluorophores typically contain several combined aromatic groups, or plane or cyclic molecules with several π bonds.
- Generally covalently bonded to a macromolecule, serving as a marker (or dye, or tag, or reporter) for affine or bioactive reagents (antibodies, peptides, nucleic acids).
- Fluorophores are notably used to stain tissues, cells, or materials in a variety of analytical methods.



Steven S. Sattlerman

Fluorophore Characteristics


- **Maximum excitation and emission wavelength** (nm):
 - Corresponds to the peak in the excitation and emission
- **Extinction Coefficient** ($\text{Mol}^{-1}\text{cm}^{-1}$):
 - Links the quantity of absorbed light, at a given wavelength, to the concentration of fluorophore in solution.
- **Quantum yield** (emitted/absorbed photons):
 - Efficiency of the energy transferred from incident light to emitted fluorescence
- **Lifetime** (in picoseconds):
 - Duration of the excited state of a fluorophore before returning to its ground state
- **Stokes shift**:
 - Difference between the max excitation and max emission wavelengths.

Steven S. Sallterman

Wikipedia.org


Introducing Molecular Beacons...

- Single-stranded oligonucleotide hybridization probes that form a stem-and-loop structure:

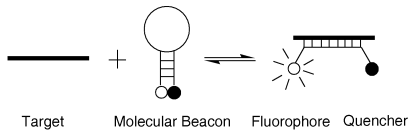

Steven S. Sallterman



Molecular Beacons...

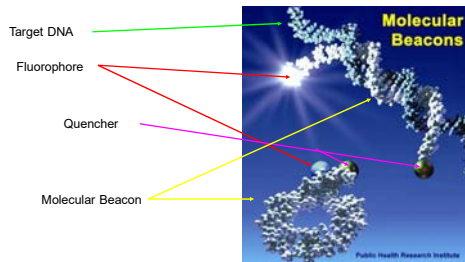

Steven S. Sallterman

Public Health Research Institute

Confocal Scanning Laser Microscopy...



Steven S. Sallerman

Image courtesy of Olympus

Chemiluminescence


- **Chemiluminescence** (CL) is the generation of light (visible, ultraviolet and infrared) by the release of energy from a chemical reaction.
- **Advantages:**
 - No excitation source (as does fluorescence and phosphorescence),
 - Only a single light detector such as a photomultiplier tube,
 - No monochromator and often not even a filter.
- Detection limits can be 10 to 100 times lower than other luminescence techniques.
- **Peroxyoxalates** are esters formed by the reaction of hydrogen peroxide and oxalate esters.

Steven S. Sallerman

Chastain, TG

Peroxyoxalate Chemiluminescence

- **Peroxyoxalate** "light-stick" reaction and emission from the reaction of **luminol** with **hydrogen peroxide** in basic aqueous solution catalyzed by **cobalt II**:




Steven S. Sallerman

Image courtesy of Simon W. Lewis, Deakin University

Surface Plasmon Resonance


- Resonant oscillation of conduction electrons at the interface between a negative and positive permittivity material stimulated by incident light.
- Detection is possible because adsorbing molecules cause changes in the local index of refraction, changing the resonance conditions of the surface plasmon waves.

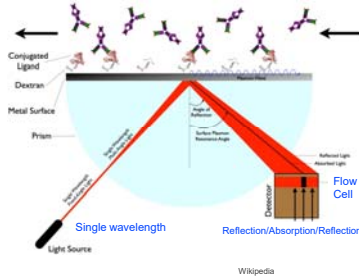

Steven S. Sallierman

Wikipedia


SPR...

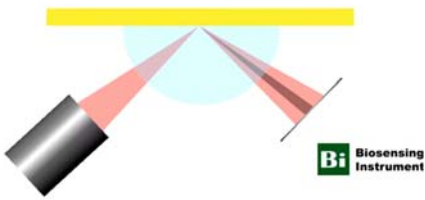

Steven S. Sallierman

<https://youtu.be/sM-VI3aWAI>

What are Surface Plasmons?

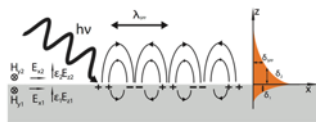

- Coherent delocalized electron oscillations that exist at the interface between any two materials.
- Surface plasmon polaritons are surface electromagnetic waves that propagate in a direction parallel to the metal/dielectric (or metal/vacuum) interface.
- Since the wave is on the boundary of the metal and the external medium (air or water for example), these oscillations are very sensitive to any change of this boundary, such as the adsorption of molecules to the metal surface

Steven S. Sallierman

Wikipedia

Localized SPR Explained...


- **Localized surface plasmon resonance (LSPR) spectroscopy** of metallic nanoparticles is a powerful technique for chemical and biological sensing experiments
- **Materials that possess a negative real and small positive imaginary dielectric constant** are capable of supporting a surface plasmon resonance (SPR).
- **Plasmonics** is the study of these particular light-matter interactions

Steven S. Sallerman

Willels, Katherine A. And RP Van Duyne. Localized surface plasmon resonance spectroscopy and sensing
Annu. Rev. Phys. Chem. 2007. 58:267-97

"Localized" Surface Plasmon Resonance

- Basis for measuring adsorption of material onto planar metal (typically gold and silver) surfaces or onto the surface of metal nanoparticles.
 - **Surface plasmon polariton (or propagating plasmon).**
 - **Localized surface plasmon.** Light interacts with particles much smaller than the incident wavelength.
- This leads to a plasmon that oscillates locally around the nanoparticle with a frequency known as the LSPR. Similar to the SPR, the LSPR is sensitive to changes in the local dielectric environment.



Steven S. Sallerman


Willels, Katherine A. And RP Van Duyne. Localized surface plasmon resonance spectroscopy and sensing
Annu. Rev. Phys. Chem. 2007. 58:267-97

Optical Detection: On-Chip

- Frequency Specific LEDs
- Absorbance Spectroscopy
- Fluorescence
- Chemiluminescence
- Optical Waveguides
- Surface Plasmon Resonance
- Interferometry
- Holography

Steven S. Sallerman


Introducing LEDs...

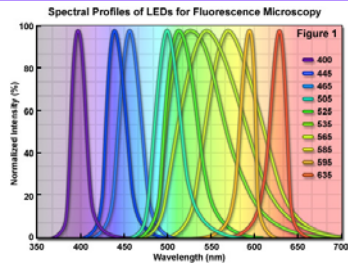

Steven S. Satterman

Image Courtesy of Zeiss

Absorbance Spectroscopy On-Chip




Increasing optical path length by making the light pass axially between parallel 45 degree mirrors.

Noda T, Takao H, Yoshioka K, Oku N, Ashiki M, Sawada K, Matsumoto K, Ishida M(2006) *Sens Actuators B* 119:245-250
 Gu, Hongwei, Yongjun Li, and Edward S. Yeung. 2011. Optical Detection Systems on Microfluidic Chips. *Microfluidics: Technologies and Applications* 304, 171-201.

Steven S. Satterman

Fluorescence




Conceptual design of a fluorescence based detection device showing a light source (LED), photodetector (CMOS), polarizers and O₂ sensitive PtOEP film arranged in a portable O₂ sensing system.

Shen, L., Ratterman, M., Klotzkin, D., Papadoukas, I. A CMOS optical detection system for point-of-use luminescent oxygen sensing. *Sens. Actuators B Chem.* 2011, 155, 430-435.

Steven S. Satterman

Chemiluminescence



Integrated opto-microfluidic sensor with a hydrogenated amorphous silicon (a-Si:H) photodetector prepared onto a glass substrate covered by a transparent conductive oxide (TCO) film.

Caputo, D., de Cesare, G., Doki, L.S., Mirasoli, M., Nassetti, A., Roda, A., Scipinotti, R. Microfluidic chip with integrated a-Si:H photodiodes for chemiluminescence-based bioassays. IEEE Sens. J. 2013, 13, 2595-2602.

Steven S. Sallerman


Waveguides for LOC based on Refractive Index

- Solid-state waveguides.**
 - Solid fibers (silica, glass or polymer) enter the chip and intersect the fluidic channel, exciting analytes and collecting the response.
- Liquid-core waveguides (LCWs).**
 - The microchannel not only transports the sample, but also transmits the light.
 - If liquid (particularly water in a microfluidic chip, with refractive index of 1.33) is used as the core of waveguide, the refractive indices of the cladding should be smaller.
- Liquid-core/liquid-cladding (L²) waveguides**
 - Two or more different laminar liquids of different refractive index flowing inside a fluidic channel.
 - The index of the cladding liquid is smaller than that of the core liquid so that the light is guided in the channel by the total internal reflection.

Gai, Hongwei, Yongjun Li, and Edward S. Yeung. 2011. Optical Detection Systems on Microfluidic Chips. Microfluidics: Technologies and Applications 304, 171-201.

Steven S. Sallerman

Liquid-Core/ Cladding (L²) Waveguide




Three parallel waveguides formed with liquid core and cladding in laminar flow systems. The direction of the light propagation can be altered by different flow rates of the adjacent fluids.

Gai, Hongwei, Yongjun Li, and Edward S. Yeung. 2011. Optical Detection Systems on Microfluidic Chips. Microfluidics: Technologies and Applications 304, 171-201.
Ligier FS (2008) Anal Chem 81:519-528

Steven S. Sallerman

Surface Plasmon Resonance On-Chip


Coupling schemes of incident light to surface plasmons.

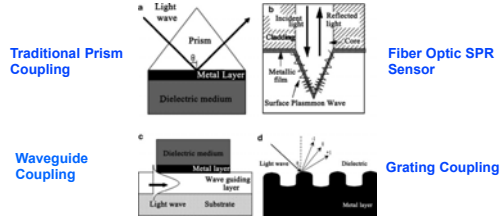

Steven S. Sallterman

Genoglu, Aydog, and Adrienne R. Minerick. 2014. Electrochemical detection techniques in micro- and nanofluidic devices. *Microfluidics and Nanofluidics* 17, no. 5:781-807.


Recall Interferometry...

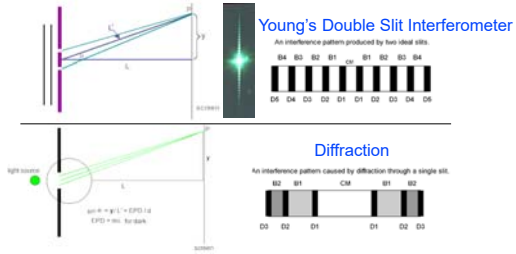

Steven S. Sallterman

Physics Lab Online and Lenox Laser


Mach-Zehnder Interferometer (MZI)

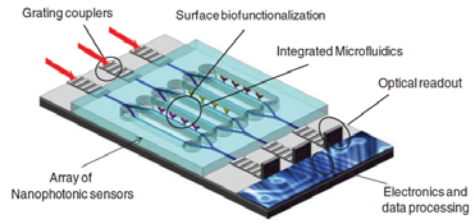

Steven S. Sallterman

Gonzalez-Guerrero, A. B., et al. 2011. Advanced photonic biosensors for point-of-care diagnostics. *Electronics* 10: 26.

Digital In-Line Holographic Microscope

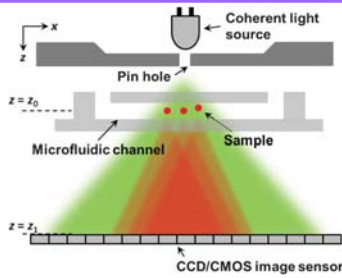

Steven S. Sallerman

Wu, J. et al. Optical imaging techniques in microfluidics and their application. Lab Chip, 2012, 12, 3566-3575

Summary

- Electrochemical Detection
 - Capillary electrophoresis.
 - Electrochemical impedance spectroscopy (EIS).
- Optical Detection
 - Conventional Off-Chip or "Free-Space"
 - Absorbance Detection
 - Fluorescence Detection
 - Chemiluminescence
 - Surface Plasmon Resonance
 - Surface Enhanced Raman Spectroscopy
 - On-Chip Methods
 - Frequency Specific LEDs
 - Absorbance Spectroscopy
 - Fluorescence
 - Chemiluminescence
 - Optical Waveguides
 - Surface Plasmon Resonance
 - Interferometry
 - Holography
 - Appendix
 - Tables of optical detection methods

Steven S. Sallerman

Table of Chemiluminescence Detection

Optical Detection	Sensor Technology	Analyte	Assay Type	Time of Analysis	Resolution	Point of Care ^a	Ref.
Chemiluminescence	Microplate reader	Hepatitis B antigen	Capillary immunoassay	25 min	0.3 ng/mL	+	[52]
Chemiluminescence	PMT	Carcinoembryonic antigen	Sandwich immunoassay	-	20 pg/mL	+	[53]
Chemiluminescence	CCD camera	Staphylococcal enterotoxin B	Sandwich immunoassay	>60 min	0.1 ng/mL	+	[54]
Chemiluminescence	Inorganic photodiodes	Anti-HRP antibody	HRP-horseradish peroxidase reaction	>60 min	0.2 nM	++	[55]
Chemiluminescence	Inorganic photodiodes	Streptavidin	HRP-horseradish peroxidase reaction	Real time	4.76 nM	++	[56]
Chemiluminescence	Organic photodiodes	Staphylococcal enterotoxin B	Sandwich immunoassay	60-70 s	0.5 ng/mL	+++	[57]

Steven S. Sallerman

Pires, NM, et al. Recent Developments in Optical Detection Technologies in Lab-on-a-Chip Devices for Biosensing Applications. Sensors 2014, 14, 15458-15479

- 52. Xiang, A.; Wei, F.; Lei, X.; Liu, Y.; Guo, Y. A simple and rapid capillary chemiluminescence immunoassay for quantitatively detecting human serum HBsAg. *Eur. J. Clin. Microbiol. Infect. Dis.* **2013**, *32*, 1557–1564.
- 53. Hao, M.; Ma, Z. An ultrasensitive chemiluminescence biosensor for carcinoembryonic antigen based on autocatalytic enlargement of immunogold nanopores. *Sensors* **2012**, *12*, 17320–17329.
- 54. Yang, M.; Sun, S.; Kostov, Y.; Rasooly, A. An automated point-of-care system for immunodetection of staphylococcal enterotoxin B. *Anal. Biochem.* **2011**, *416*, 74–81.
- 55. Caputo, D.; de Cesare, G.; Dolci, L.S.; Mirasoli, M.; Nascetti, A.; Roda, A.; Scipinotti, R. Microfluidic chip with integrated a-Si:H photodiodes for chemiluminescence-based bioassays. *IEEE Sens. J.* **2013**, *13*, 2595–2602.
- 56. Lin, C.C.; Ko, F.H.; Chen, C.C.; Yang, Y.S.; Chang, F.C.; Wu, C.S. Miniaturized metal semiconductor metal photocurrent system for biomolecular sensing via chemiluminescence. *Electrophoresis* **2009**, *30*, 3189–3197.
- 57. Wojciechowski, J.R.; Shriver-Lake, L.C.; Yamaguchi, M.Y.; Füreder, E.; Pieler, R.; Schamesberger, M.; Winder, C.; Prall, H.J.; Sonnleitner, M.; Ligler, F.S. Organic photodiodes for biosensor miniaturization. *Anal. Chem.* **2009**, *81*, 3455–3461.

Steven S. Sallterman

Table of Fluorescence Detection

Optical Detection	Sensor Technology	Analyte	Assay Type	Time of Analysis	Resolution	Point of Care ^a	Ref.
Fluorescence	CMOS image sensor	<i>Giardia Lamblia</i> cysts	Microscopy	~1 s	Focal plane of 0.8 μm	-	[41]
Fluorescence	CCD camera	Bacterial DNA	PCR	Real time	~50 CFU/mL ^b	+	[49]
Fluorescence	Inorganic photodiodes	17-β estradiol	Competitive aptamer assay	~10 min	0.6 ng/mL	++	[50]
Fluorescence	Organic photodiodes	Alkylphenol polyethoxylates	Competitive immunoassay	~5 min	2–4 ppb	++	[51]


Prasanna, M.M. et al. Recent Developments in Optical Detection Technologies in Lab-on-a-Chip Devices for Biosensing Applications. *Sensors* 2014, *14*, 15458–15479

Steven S. Sallterman

- 41. Lee, L.M.; Cui, X.; Yang, C. The application of on-chip optofluidic microscopy for imaging *Giardia lamblia* trophozoites and cysts. *Biomed. Microdevices* **2009**, *11*, 951–958.
- 49. Ramalingam, N.; Rui, Z.; Liu, H.B.; Dai, C.C.; Kaushik, R.; Ratnahrarka, B.M.; Gong, H.Q. Real-time PCR-based microfluidic array chip for simultaneous detection of multiple waterborne pathogens. *Sens. Actuators B Chem.* **2010**, *145*, 543–552.
- 50. Yildirim, N.; Long, F.; Gao, C.; He, M.; Shi, H.C.; Gu, A.Z. Aptamer-based optical biosensor for rapid and sensitive detection of 17β-estradiol in water samples. *Environ. Sci. Technol.* **2012**, *46*, 3288–3294.
- 51. Ishimatsu, R.; Naruse, A.; Liu, R.; Nakano, K.; Yahiro, M.; Adachi, C.; Imato, T. An organic thin film photodiode as a portable photodetector for the detection of alkylphenol polyethoxylates by a flow fluorescence-immunoassay on magnetic microbeads in a microchannel. *Talanta* **2013**, *117*, 139–145.

Steven S. Sallterman

SPR Sensing Approach

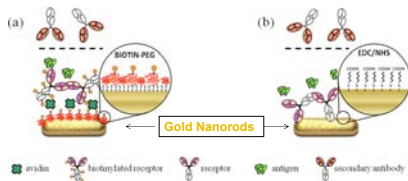


Schematic of the sensing approaches used for the detection of the analyte of interest where :
 a) A biotin-avidin is used to link the receptor.
 b) Carbodiimide chemistry is used.

Steven S. Sallterman

Acimovic, SS. LSPR Chip for Parallel, Rapid, and Sensitive Detection of Cancer Markers in Serum. *Nano Lett.* 2014, 14, 2636-2641

Example: Cancer Marker Detection – Acimovic et. al.


Gold Nanorod Array

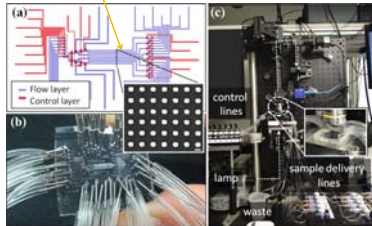

Steven S. Sallterman

Acimovic, SS. LSPR Chip for Parallel, Rapid, and Sensitive Detection of Cancer Markers in Serum. *Nano Lett.* 2014, 14, 2636-2641

Detection of AFP and PSA Markers

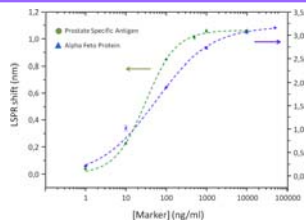

Parallel biosensor chip (LSPR response) for the detection of AFP and PSA cancer markers in 50% human serum.

Steven S. Sallterman

Acimovic, SS. LSPR Chip for Parallel, Rapid, and Sensitive Detection of Cancer Markers in Serum. *Nano Lett.* 2014, 14, 2636-2641
